


REPORT

Sequence :

:

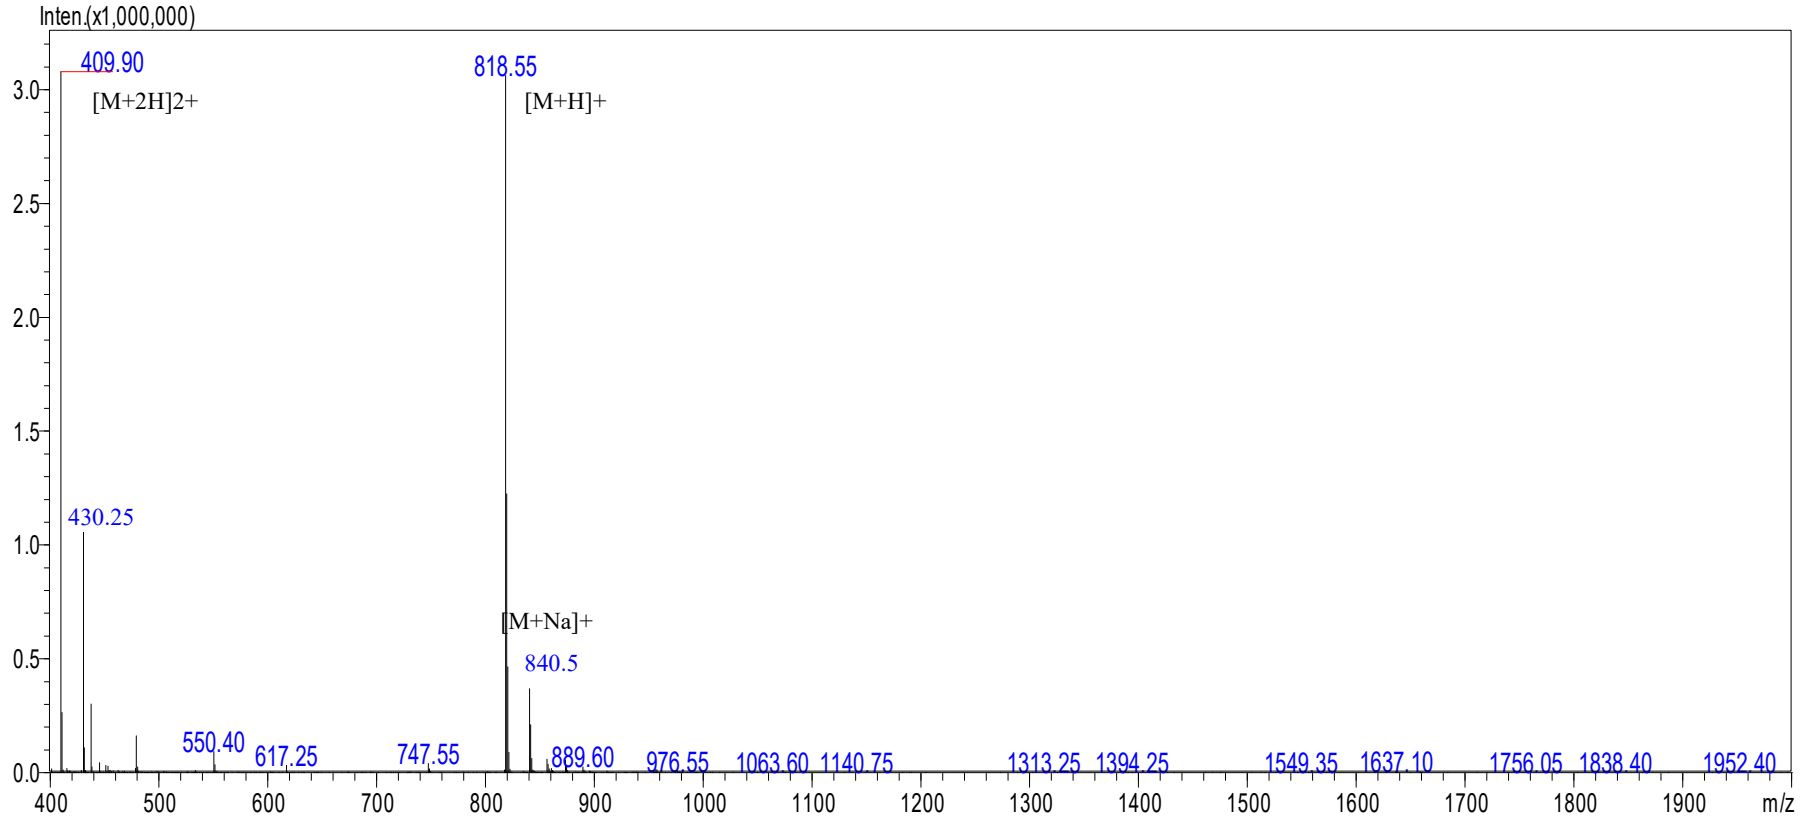

Date and Time: 2018-11-18 10:41:30
User : CHAO
Sample : GHRP-2
MW : 818.0
Lot No. : P181118-VZ055255

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp: 250°C
Block Temp: 200°C

Probe bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. conc: 50%H₂O/50%ACN