


REPORT

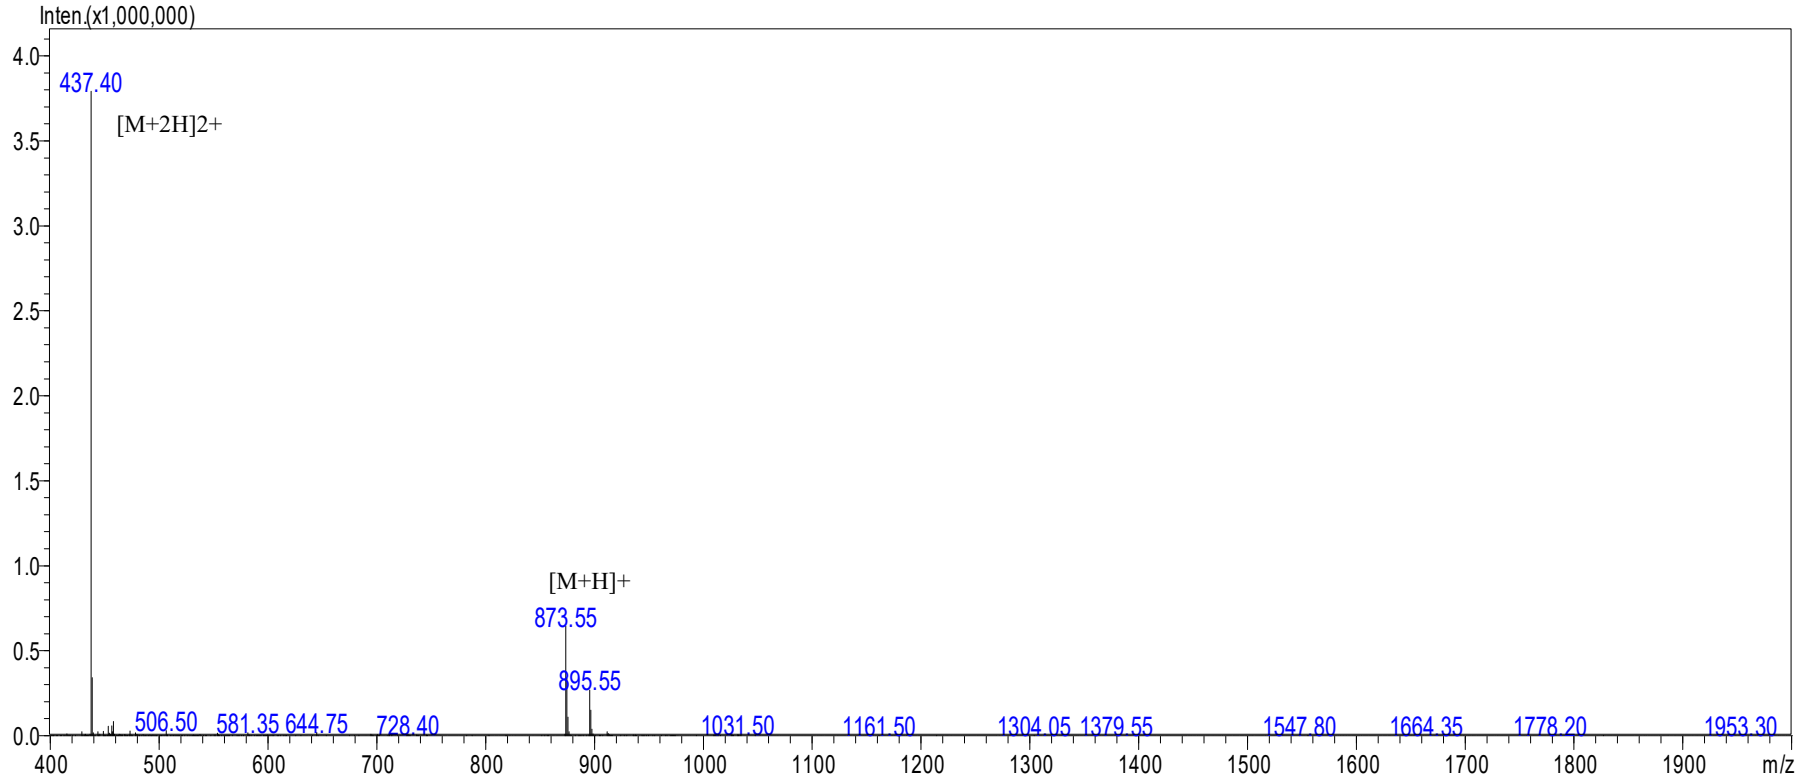

Date and Time: 2018-11-14 14:21:42
User : CHAO
Sample : GHRP-6
MW : 873.04
Lot No. : P181114-VZ055254

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp: 250°C
Block Temp: 200°C

Probe bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. conc: 50%H₂O/50%ACN