


REPORT

Sequence :

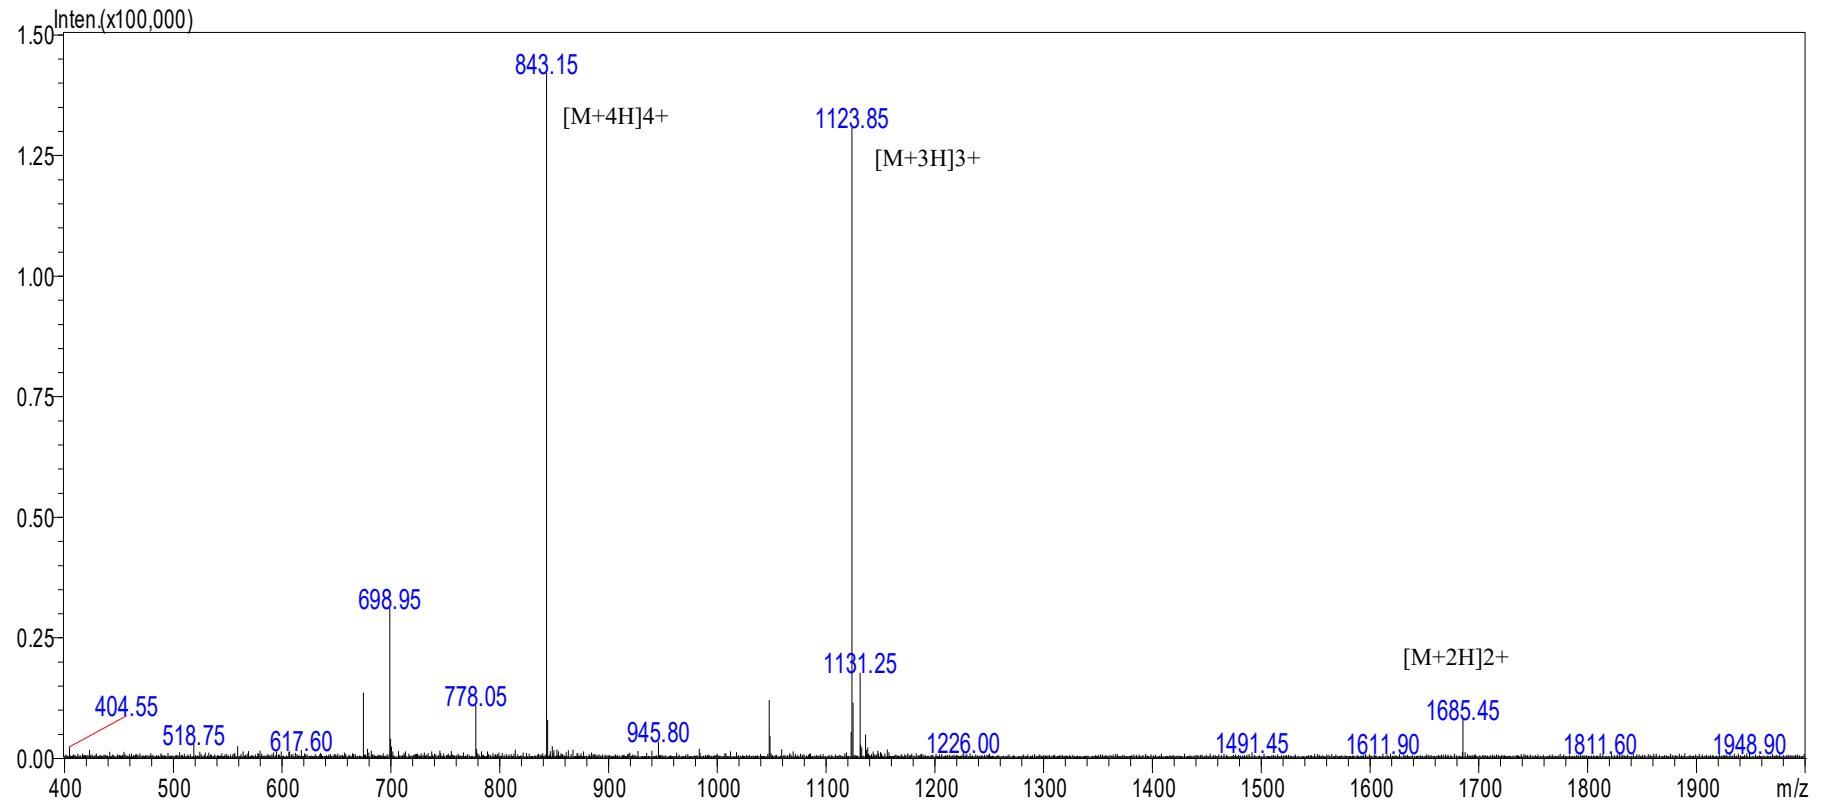

Date and Time: 2018-11-27 16:10:22  
User : CHAO  
Sample : CJC-1295  
MW : 3367.97  
Lot No. : P181127-VZ088421

Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp: 250°C  
Block Temp: 200°C

Probe bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. conc: 50%H2O/50%ACN